

10-31-2017

# Assessing the reliability of ultrasound imaging to examine peripheral nerve excursion: A systematic literature review

Ben Kasehagen  
*Bond University*

Richard Ellis  
*Auckland University of Technology*

Rodney Pope  
*Bond University*

Nicholas Russell  
*Bond University*

Follow this and additional works at: [http://epublications.bond.edu.au/hsm\\_pubs](http://epublications.bond.edu.au/hsm_pubs)

Wayne Hing  
 Part of the [Analytical, Diagnostic and Therapeutic Techniques and Equipment Commons](#), and the [Radiology Commons](#)



This work is licensed under a [Creative Commons Attribution-Noncommercial-No Derivative Works 4.0 License](#).

## Recommended Citation

Kasehagen, B., Ellis, R., Pope, R., Russell, N., & Hing, W. (2017). Assessing the reliability of ultrasound imaging to examine peripheral nerve excursion: A systematic literature review. Retrieved from <https://doi.org/10.1016/j.ultrasmedbio.2017.08.1886>

This Journal Article is brought to you by the Faculty of Health Sciences & Medicine at [ePublications@bond](#). It has been accepted for inclusion in Faculty of Health Sciences & Medicine Publications by an authorized administrator of [ePublications@bond](#). For more information, please contact [Bond University's Repository Coordinator](#).



● *Review*

## ASSESSING THE RELIABILITY OF ULTRASOUND IMAGING TO EXAMINE PERIPHERAL NERVE EXCURSION: A SYSTEMATIC LITERATURE REVIEW

BEN KASEHAGEN,\* RICHARD ELLIS,† RODNEY POPE,\* NICHOLAS RUSSELL,\* and WAYNE HING\*

\* Bond Institute of Health and Sport, Faculty of Health Sciences and Medicine, Bond University, Robina, Gold Coast, Queensland, Australia; and † Health and Rehabilitation Research Institute, School of Clinical Sciences, Auckland University of Technology, Auckland, New Zealand

(Received 29 March 2017; revised 22 August 2017; in final form 28 August 2017)

**Abstract**—Ultrasound imaging (USI) is gaining popularity as a tool for assessing nerve excursion and is becoming an important tool for the assessment and management of entrapment neuropathies. This systematic review aimed to identify current methods and report on the reliability of using USI to examine nerve excursion and identify the level of evidence supporting the reliability of this technique. A systematic search of five electronic databases identified studies assessing the reliability of using USI to examine nerve excursion. Two independent reviewers critically appraised and assessed the methodological quality of the identified articles. Eighteen studies met the eligibility criteria. The majority of studies were of “moderate” or “high” methodological quality. The overall analysis indicated a “strong” level of evidence of moderate to high reliability of using USI to assess nerve excursion. Further reliability studies with consistency of reporting are required to further strengthen the level of evidence. (E-mail: [benkasehagen@gmail.com](mailto:benkasehagen@gmail.com)) © 2017 Published by Elsevier Inc. on behalf of World Federation for Ultrasound in Medicine & Biology. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

**Key Words:** Reliability, Nerve excursion, Ultrasound imaging.

### INTRODUCTION

The peripheral nervous system is constantly exposed to mechanical loads imposed upon it by movements and postures of the body. To cope with and respond to these external forces (tensile, shear and compressive forces), a peripheral nerve must be able to withstand compression, elongate and stretch, glide and slide relative to its interfacing tissues (Topp and Boyd 2012). Compromise of any one (or combination) of these neural biomechanical responses is believed to be part of the multifactorial etiology of many peripheral neuropathies (Dilley et al. 2008; Greening et al. 2005). For example, one of the most commonly reported features of carpal tunnel syndrome is impaired median nerve movement through the carpal tunnel or forearm (Filius et al. 2013; Hough et al. 2007; Nakamichi and Tachibana 1995). A recent systematic review concluded that reduced median nerve excursion, observed with ultrasound imaging (USI), was a commonly reported and

significant feature of carpal tunnel syndrome (Ellis et al. 2017).

With this in mind, the assessment of nerve biomechanics is rapidly evolving, with *in vivo* methods superseding traditional cadaveric methods. For example, contemporary methods for evaluating peripheral nerve excursion *in vivo* utilize real-time USI. A range of research reports have detailed the use of USI to assess *in vivo* nerve excursion for the median (Coppieters et al. 2009; Dilley et al. 2003; Filius et al. 2013; Hough et al. 2007), ulnar (Dilley et al. 2007), radial (Kasehagen et al. 2016), sciatic (Coppieters et al. 2015; Ellis et al. 2012; Ridehalgh et al. 2012), tibial (Carroll et al. 2012; Ellis et al. 2008) and common fibular (Boyd et al. 2012) nerves. Newer technologies, such as sonoelastography, have been reported as methods to examine nerve excursion and also parameters such as shear strain and passive stiffness (Andrade et al. 2016; Greening and Dilley 2017; Yoshii et al. 2017). Furthermore, USI can also be used to assess peripheral nerve morphology and structure (*e.g.*, thickness and cross-sectional area) (Alshami et al. 2009; Fink et al. 2017).

On this basis, there exists a significant opportunity to utilize USI to assess peripheral nerve structure and excursion in clinical populations, particularly those with

Address correspondence to: Ben Kasehagen, Bond Institute of Health and Sport, Faculty of Health Sciences and Medicine, Bond University, Robina, Gold Coast, Queensland 4226, Australia. E-mail: [benkasehagen@gmail.com](mailto:benkasehagen@gmail.com)

peripheral neuropathies. There is growing support for diagnostic use of USI to evaluate nerve biomechanics and structure in clinical conditions such as carpal tunnel syndrome (Ellis et al. 2017; McDonagh et al. 2015). However, the expansion of these *in vivo* techniques for use in clinical populations is still in its infancy.

For researchers and clinicians to have confidence in using USI to assess *in vivo* nerve excursion, the available methods need to have been assessed to confirm adequate levels of measurement reliability. Furthermore, the growing popularity, cost effectiveness and accessibility of USI highlights the importance of determining its reliability when used for such measurements. On this basis, the purpose of this systematic review was to identify, critically appraise and synthesize key findings from studies that have assessed the reliability of USI measurements of peripheral nerve excursion *in vivo*. The specific aims of the review were to identify those peripheral nerves that have been examined in this way, to document the approaches used for making such measurements, to investigate the reported levels of reliability for these measurements while considering the methodological quality of the identified reliability studies and to establish the current level of evidence that supports the reliability of using USI to quantify nerve excursion. The scope of the review was limited to examining nerve excursion and does not include examination of any other biomechanical properties of the nerve.

## METHODS

The design and reporting of this systematic review with critical narrative synthesis have been guided by the Centre for Reviews and Dissemination's Guidance for Undertaking Reviews in Health Care (Centre for Reviews and Dissemination 2009) and the Preferred Reporting Items for Systematic Reviews and Meta-analyses (PRISMA) statement (Moher et al. 2009).

### Search strategy

A systematic literature search was conducted to identify all relevant articles for inclusion in this review. The search sought articles published up until May 2016, with no restriction on publication date. The search was conducted across the relevant health and science electronic databases (PubMed, Embase, CINAHL, SportDiscus and Scopus), with additional hand searching of reference lists of eligible articles also performed. The search was conducted using a consistent search strategy across all databases and included key words from three main concepts: USI (ultrasound, ultrasonography, sonography), reliability (reliability, repeatability) and nerve excursion (nerve, peripheral nerve, nervous system, neural system, nerve movement, nerve excursion, neurodynamic, neural mo-

bilization, neural mobilization, neural glide, nerve glide, neural slide, nerve slide). The Boolean operators "Or" and "And" were used to link the key words from each concept and to link the concepts themselves, respectively. After article selection, a final hand search was performed of the reference lists of the included articles to identify any other potentially eligible articles.

### Screening and selection

One reviewer (B.K.) screened all titles and abstracts of the 1592 articles identified in the literature search to assess potential eligibility. Duplicates (151) and articles that were clearly ineligible (1412) were excluded during this initial screening process. Full text was obtained of the remaining 29 potentially eligible studies. One of these 29 studies was reported in two separate articles (Ridehalgh et al. 2012, 2014); these articles utilized the same participant group and were therefore considered within the remainder of this systematic review in reference to the original work (Ridehalgh et al. 2012).

Two reviewers (B.K. and N.R.) independently appraised all identified studies against the following inclusion and exclusion criteria to determine final eligibility. Differences in judgments were discussed with an additional reviewer (R.E.), who acted as an arbiter to determine the final judgment of eligibility.

### Inclusion criteria

Ultrasound imaging was used to quantify *in vivo* nerve excursion. Reliability of assessing nerve excursion was quantified, and the method of statistical analysis used to assess reliability was specified.

The sample included human participants; no restrictions were made regarding type of study cohort (*e.g.*, healthy or clinical populations).

Informed consent was provided for all study participants, as was protocol approval by an ethics committee or institutional review board.

### Exclusion criteria

*Articles not available in English or full text not available.* Those studies deemed eligible formed the final set of included studies for the review. The results of the search, screening and selection processes were documented in a PRISMA diagram (Fig. 1) (Moher et al. 2009).

*Critical appraisal of methodological quality.* The methodological quality of all included studies was critically appraised using a standardized Critical Appraisal Tool (CAT) developed by Brink and Louw (2012). The CAT was designed specifically to critically appraise the methodological quality of reliability and validity studies that have assessed clinical outcome measures and objective tests (Brink and Louw 2012). The CAT consists of 13 items in

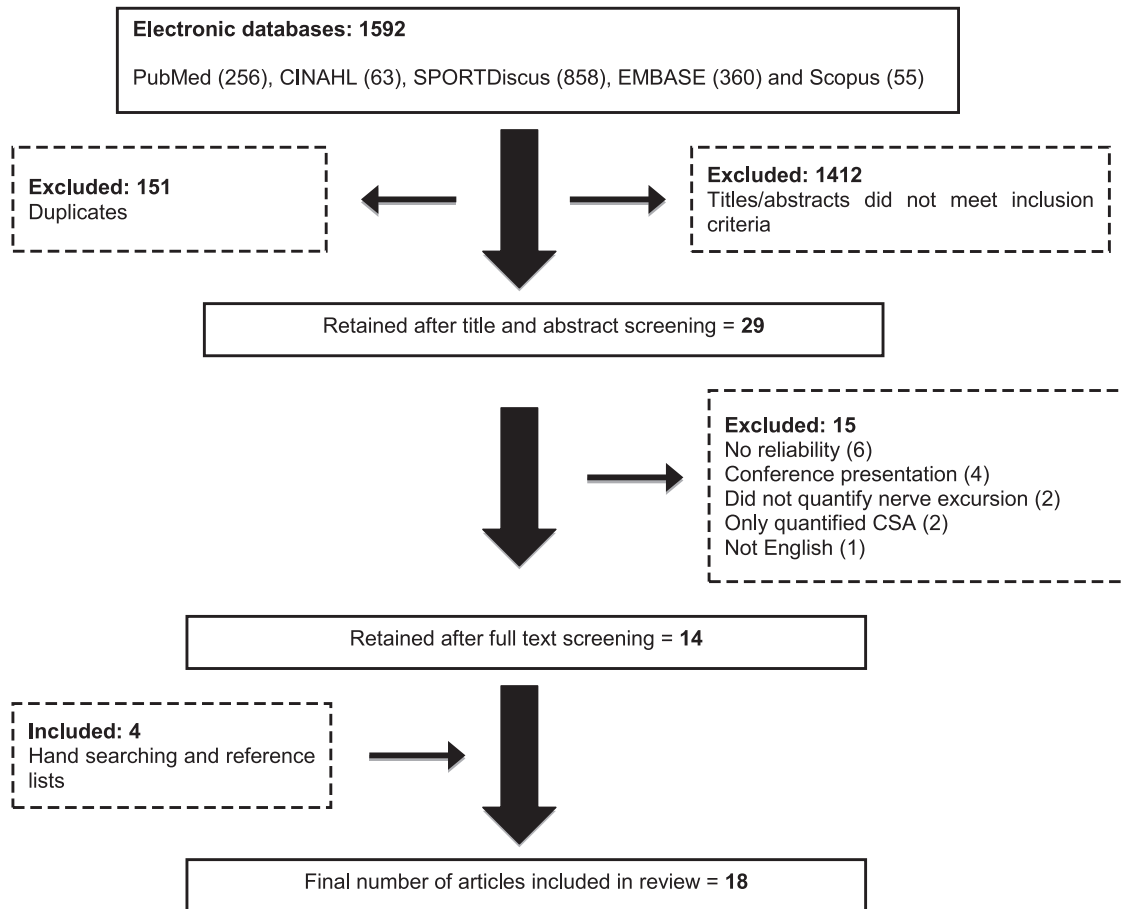


Fig. 1. Preferred Reporting Items for Systematic Reviews and Meta-analyses (PRISMA) flow diagram.

total, some of which are pertinent to assessing reliability methods and some of which are pertinent to assessing clinical validity methods. As previously reported (Rabelo *et al.* 2015), four items of the CAT (items 3, 7, 9 and 11) are relevant only to methods used to assess validity; therefore, these items were excluded from use in the current review. This left a total of nine items to be used in the modified CAT (MCAT) for appraising the methodological quality of the included studies. From these items, both items 4 and 5 relate to blinding of the raters—to either the findings of other raters (item 4, inter-rater reliability) or to their own findings (item 5, intra-rater reliability) (Brink and Louw 2012). With this in mind, for this review, items 4 and 5 of the MCAT were combined to form a single item to be assessed, with an overall score of “yes” or “no” being awarded depending on whether blinding of raters was reported in a way that was appropriate to the particular study design (*i.e.*, based on whether the study assessed inter-rater reliability, intra-rater reliability or both).

The CAT developed by Brink and Louw (2012) does not yield an overall quality score or rating, and therefore, a scoring and rating system previously developed by

Prowse *et al.* (2016) for use with this MCAT was employed. One point was awarded for meeting each item of the MCAT, with a maximum score of eight points possible, as items 4 and 5 were combined to form one item. Methodological quality ratings were then assigned as follows, based on total quality score: 0–2 = poor; 3–4 = fair; 5–6 = moderate; and 7–8 = high (Prowse *et al.* 2016). Two reviewers (B.K. and N.R.) independently appraised all identified studies using the MCAT. Differences in judgments for individual items were discussed with a third reviewer (R.P.), who acted as an arbiter to determine a final judgment for the item.

#### Data extraction and analysis

Methodological details and key findings of relevance to the aim of this review were extracted from each included study using a systematic approach and then tabulated to allow for comparisons across the included studies. Meta-analysis was not performed because of the heterogeneity of the different methods employed across the included studies (*e.g.*, differences in the nerves examined, the body sites selected for USI and the body

Table 1. Levels of evidence approach

Level of evidence	Criterion
<b>Strong</b>	Consistent findings from greater than three high-quality studies
<b>Moderate</b>	Consistent findings from at least one high-quality and one or more low-quality studies
<b>Limited</b>	Consistent findings in one low-quality study or only one study available
<b>Conflicting</b>	Inconsistent evidence in multiple studies irrespective of study quality

Source. van Tulder et al. (2003).

movements utilized to induce nerve movement). Instead, descriptive analysis and a critical narrative synthesis of key findings were performed.

After data extraction and tabulation, a descriptive analysis was conducted to determine the levels of evidence provided by the included studies regarding the reliability of USI measurements of nerve excursion (van Tulder et al. 2003). This approach to assessing levels of evidence has been used in other systematic reviews (Barrett et al. 2014; Prowse et al. 2016). During this analysis, for each nerve imaged in the included studies, a rating was assigned to reflect the level of evidence provided by the included studies that related to that particular nerve. The level of evidence in each instance was rated as strong, moderate, limited or conflicting based on the number of relevant studies, along with the methodological quality, and using the rating system reported by van Tulder et al. (2003) (Table 1).

A critical narrative synthesis was then conducted, first to elucidate commonalities and variations in the protocols used in the different studies and for different nerves to measure nerve excursion using USI. This was important, because the reliability of measurements can clearly be affected by the measurement protocol. Second, the critical narrative synthesis considered the key findings from included studies regarding the reliability of USI measurements of nerve excursion. The synthesis considered reliability of these measurements for each nerve specifically and overall.

## RESULTS

### *Literature search and selection*

Results of the literature search, screening and selection processes are summarized in the PRISMA diagram in Figure 1. Eighteen studies, including four studies identified from manual searching of the reference lists of eligible studies, met the eligibility criteria and were included in the final review. The study conducted by Ridehalgh et al. (2014) reported reliability data that were previously presented by the same group in 2012 (Ridehalgh et al. 2012). For this reason, the data reported in Ridehalgh et al. (2012)

were reported in the current review without further inclusion of the 2014 study.

### *Peripheral nerves examined*

Of the 18 studies included in this review, 9 examined the median nerve (Coppieters et al. 2009; Farooq 2012; Filius et al. 2013; Gonzalez-Suarez et al. 2015; Hough et al. 2000, 2007; Martínez-Payá et al. 2015; Paquette et al. 2015; Wang et al. 2014), 1 examined the radial nerve (Kasehagen et al. 2016), 4 examined the sciatic nerve (Coppieters et al. 2015; Ellis et al. 2008, 2012; Ridehalgh et al. 2012), 5 examined the tibial nerve (Boyd and Dilley 2014; Boyd et al. 2012; Carroll et al. 2012; Ellis et al. 2008; Shum et al. 2013) and 1 examined the common fibular nerve (Boyd et al. 2012).

### *Participant characteristics*

A total of 392 participants were involved across the 18 studies included in the current review, with 59% of these participants being female. The sample sizes in individual studies ranged from 6 participants (Gonzalez-Suarez et al. 2015) to 56 participants (Hough et al. 2007). The average age across all groups was 36 y (range: 18–86 y).

Thirteen studies recruited solely healthy participants (Carroll et al. 2012; Coppieters et al. 2009, 2015; Ellis et al. 2008, 2012; Filius et al. 2013; Gonzalez-Suarez et al. 2015; Hough et al. 2000; Kasehagen et al. 2016; Martínez-Payá et al. 2015; Ridehalgh et al. 2012; Shum et al. 2013; Wang et al. 2014). Four studies compared healthy participants with participants with known clinical conditions, which included type II diabetes mellitus (Boyd et al. 2012), type I or type II diabetes mellitus (Boyd and Dilley 2014), whiplash-associated disorder (Farooq 2012) and carpal tunnel syndrome (Hough et al. 2007). The remaining study pooled the data from healthy and carpal tunnel syndrome participants and did not compare between groups (Paquette et al. 2015). See Table 2 for further participant information.

### *Protocols for USI measurements of nerve excursion*

A number of different protocols and techniques have been reported for using USI to quantify nerve excursion. The most commonly reported is frame-by-frame digital analysis of grey speckle features from within the ultrasound image (also known as speckle tracking). Several different software packages have been reported that use cross-correlation algorithms to compare the movement of gray-scale, speckle features (within specified regions of interest) between individual ultrasound frames (Dilley et al. 2001; Nicoud et al. 2011). Thirteen of the 18 included studies (Boyd and Dilley 2014; Boyd et al. 2012; Carroll et al. 2012; Coppieters et al. 2009, 2015; Ellis et al. 2008, 2012; Farooq 2012; Gonzalez-Suarez et al. 2015; Kasehagen et al. 2016; Paquette et al. 2015; Ridehalgh et al.

Table 2. Modified Critical Appraisal Tool of reliability studies (MCAT)

Study	Study population		Testing circumstances and execution					Data analysis	Quality	
Reference	Study sample	Item 1 Demographic characteristics Cohort: Mean age (range)	Item 2 Adequate description of observer and competence	Items 4, 5 (combined) Intra- and/or inter-observer blinding	Item 6 Order examination varied for test condition	Item 8 Stability of variable and suitability of time interval	Item 10 Sufficient description of test procedure	Item 12 Description results with explanation withdrawals	Item 13 Appropriate statistical method	Score
<b>Median nerve</b>										
Martínez-Payá <i>et al.</i> (2015)	n = 22 11 M:11 F	Y Healthy: 22 y	Y Sonographer 12 y of USI experience	N Not stated Inter-observer	NA One test condition	N Not stated	Y	Y No withdrawals	Y κ coefficient (95% CI)	5/8 Moderate
Gonzalez-Suarez <i>et al.</i> (2015)	n = 6 2 M:4 F	Y Healthy: 24 y	Y Physician 6 y of MSK USI experience Two assessors: Rehabilitation Medicine residents	N Not stated Intra- and inter-observer	N Not stated	Y 1 h between procedures 1-d interval between assessors 1-mo measurements were repeated	Y	Y No withdrawals	Y ICC (95% CI), SEM, MDC	6/8 Moderate
Paquette <i>et al.</i> (2015)	n = 7 2 M:5 F n = 11 6 M:5 F	Y Uni/bilateral CTS: 56 y Healthy: 37 y	Y Trained physical therapist	N Not stated Intra-observer	N Not stated	Y 30-min interval	Y	Y No withdrawals	Y Dependability coefficient SEM MDC ICC (95% CI)	6/8 Moderate
Wang <i>et al.</i> (2014)	n = 10 4 M:6 F (bi-lateral wrists)	Y Healthy: 39 y	Y Radiologist 5 y MSK USI experience	N Not stated Intra- and inter-observer	N Not stated	Y ≥3 mo between analyses	Y	Y No withdrawals	Y ICC (95% CI)	6/8 Moderate
Filius <i>et al.</i> (2013)	n = 20 10 M:10 F	Y Healthy: 28 (21–72) y	Y Physician MSK USI experience	Y Blinded Intra- and inter-observer	Y Randomized	Y 2-d interval	Y	Y No withdrawals	Y ICC (95% CI)	8/8 High
Farooq (2012)	n = 7 2 M:5 F n = 10 5 M:5 F	Y WAD: 35 Healthy: 25 y	Y Trained MSK physiotherapist	N Not stated Inter-observer	NA One test condition	N Not stated	Y	Y No withdrawals	N ICC	4/7 Moderate
Coppieters <i>et al.</i> (2009)	n = 15 7 M:8 F	Y Healthy: 30	N Not stated	N Not stated Inter-observer	Y Randomized	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM, MDC	5/8 Moderate
Hough <i>et al.</i> (2007)	n = 19 8 M:11 F n = 37 8 M:29 F	Y Idiopathic CTS: 57 (35–86) y Healthy: 48 (21–64) y	N Not stated	Y Blinded Intra-observer	Y Reversed order	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM	6/8 Moderate
Hough <i>et al.</i> (2000)	n = 16 7 M:9 F (bilateral arms)	Y Healthy: 38 (26–61) y	N Not stated	Y Blinded Intra-observer	NA One test condition	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM	5/8 Moderate
<b>Radial nerve</b>										
Kasehagen <i>et al.</i> (2016)	n = 30 12 M:18 F	Y Healthy: 30 (19–49) y	Y Sonographer 10 y of USI experience	Y Blinded Intra-observer	Y Randomized	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM, MDC, Bland–Altman plot	7/8 High

(continued on next page)

Table 2. (continued)

Study	Study population		Testing circumstances and execution							Data analysis	Quality
			Item 1 Demographic characteristics Cohort: Mean age (range)	Item 2 Adequate description of observer and competence	Items 4, 5 (combined) Intra- and/or inter-observer blinding	Item 6 Order examination varied for test condition	Item 8 Stability of variable and suitability of time interval	Item 10 Sufficient description of test procedure	Item 12 Description results with explanation withdrawals		
Reference	Study sample									Score	
<b>Sciatic nerve</b>											
Coppieters et al. (2015)	n = 15 6 M:9 F	Y Healthy: 28	N Not stated	Y Blinded Inter-observer	Y Randomized	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM	6/8 Moderate	
Ridehalgh et al. (2012, 2014)	n = 18 9 M:9 F	Y Healthy: 29 (19–68) y	Y MSK physiotherapist	N Not stated Intra-observer	N Same order	Y 48 h—one wk interval	Y	Y Description of excluded data	Y ICC (95% CI), SEM, Bland-Altman plot	6/8 Moderate	
Ellis et al. (2012)	n = 31 9 M:22 F	Y Healthy: 29 (21–61) y	Y Sonographer 5 y experience	Y Blinded Intra-observer	Y Randomized	Y 1-min interval	Y	Y Description of excluded data	Y ICC (95% CI), SEM	8/8 High	
<b>Sciatic and tibial nerves</b>											
Ellis et al. (2008)	n = 27 13 M:14 F	Y Healthy: 23 (18–38)	Y Experienced sonographer	Y Blinded Intra-observer	N Not stated	Y 1-min interval	Y	Y No withdrawals	Y ICC (95% CI), SEM, Bland-Altman plot	7/8 High	
<b>Tibial nerve</b>											
Boyd and Dilley (2014)	n = 20 6 M:14 F n = 20 10 M:10 F	Y Type I and/or II DM: 51 (25–66) y Healthy: 46 (23–66) y	N Not stated	Y Blinded Intra-observer	N Not stated	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM	5/8 Moderate	
Shum et al. (2013)	n = 25 11 M:14 F	Y Healthy: 29 y	N Not stated	N Not stated Intra-observer	NA One test condition	Y 2-min interval	Y	Y Description of excluded data	Y ICC (95% CI), SEM	5/8 Moderate	
Carroll et al. (2012)	n = 16 6 M:10 F	Y Healthy: 35 y	Y Examiner 3 mo of USI training	N Not stated Intra-observer	NA One test condition	Y 1-min interval between repeated scans. 5-min interval between sessions 1 and 2	Y	Y No withdrawals	Y ICC (95% CI), SEM, SRD	6/8 Moderate	
<b>Tibial and common fibular nerves</b>											
Boyd et al. (2012)	n = 5 4 M:1 F n = 5 1 M:4 F	Y Type II DM: 57 y Healthy: 40 y	N Not stated	N Not stated Intra-observer	N Not stated	N Not stated	Y	Y No withdrawals	Y ICC (95% CI), SEM	4/8 Fair	

Y = met MCAT criteria; N = did not meet MCAT criteria; NA = not accessible; M = male; F = female; DM = diabetes mellitus; WAD = whiplash-associated disorder; CTS = carpal tunnel syndrome; ICC = intra-class correlation; CI = confidence interval; MDC = minimal detectable change; SRD = smallest real difference; SEM = standard error measurement; USI = ultrasound imaging; MSK = musculoskeletal.

2012; Shum *et al.* 2013) utilized this type of analysis method. Of these 13 studies, 12 (Boyd and Dilley 2014; Boyd *et al.* 2012; Carroll *et al.* 2012; Coppieters *et al.* 2009, 2015; Ellis *et al.* 2008, 2012; Farooq 2012; Kasehagen *et al.* 2016; Paquette *et al.* 2015; Ridehalgh *et al.* 2012; Shum *et al.* 2013) utilized the protocol of frame-by-frame cross-correlation analysis as reported initially by Dilley *et al.* (2001).

Two studies utilized real-time spectral Doppler USI to quantify nerve excursion (Hough *et al.* 2000, 2007). By measuring the deflections of the Doppler/B-mode signals, in several planes, velocity of nerve movement was calculated with excursion quantified from measuring the area under the deflection traces (Hough *et al.* 2000).

For the measurement of transverse nerve movement, several studies compared the position of the relevant nerve (often the centroid point or the nerve outline) and digitally measured the change in nerve position (representing the amount of excursion) between the first and final frames of an ultrasound video (Ellis *et al.* 2008; Filius *et al.* 2013; Martínez-Payá *et al.* 2015; Wang *et al.* 2014).

#### *Critical appraisal of methodological quality*

The methodological quality of the studies included in this review was rated as high for 4 studies (Ellis *et al.* 2008, 2012; Filius *et al.* 2013; Kasehagen *et al.* 2016), moderate for 13 studies (Boyd and Dilley 2014; Carroll *et al.* 2012; Coppieters *et al.* 2009, 2015; Farooq 2012; Gonzalez-Suarez *et al.* 2015; Hough *et al.* 2000, 2007; Martínez-Payá *et al.* 2015; Paquette *et al.* 2015; Ridehalgh *et al.* 2012; Shum *et al.* 2013; Wang *et al.* 2014) and fair for 1 study (Boyd *et al.* 2012). Across all of the included studies, the items regarding description of participant characteristics (item 1) and test procedure (item 10), explanation of withdrawals (item 12) and description of appropriate statistical analyses (item 13) were all satisfied.

There was some variability across the studies regarding the description of the level of experience or competence of the sonographer (item 2). Seven studies did not describe the person performing USI (Boyd and Dilley 2014; Boyd *et al.* 2012; Coppieters *et al.* 2009, 2015; Hough *et al.* 2000, 2007; Shum *et al.* 2013), whilst a further three studies (Farooq 2012; Paquette *et al.* 2015; Ridehalgh *et al.* 2012) stated a “trained” physiotherapist conducted the imaging, with the implication that they were trained in USI.

There was also variability in the reporting of observer (*i.e.*, rater) blinding, irrespective of whether the studies examined intra-rater reliability or inter-rater reliability (items 4 and 5 combined). Ten studies (Boyd *et al.* 2012; Carroll *et al.* 2012; Coppieters *et al.* 2009; Farooq 2012; Gonzalez-Suarez *et al.* 2015; Martínez-Payá *et al.* 2015; Paquette *et al.* 2015; Ridehalgh *et al.* 2012; Shum *et al.* 2013; Wang *et al.* 2014) did not report blinding of the observers during the data analysis.

Item 6 concerned the order in which participants were assessed on each measurement occasion. Randomization of participant order can reduce the possibility of confounding through recall of ordered participants and results. There was variability in the scores for this item across studies.

The stability of a measured variable (in this case, nerve excursion) over time (item 8) is a feature of reliability studies that should be taken into account. It is possible that calculations of the reliability of measurement may be affected not only by lack of repeatability in the measurement methods or technique, but also because the measured variable itself alters over time. In situations where the measured variable is quite unstable and rapidly changing, the interval between measurement occasions must be kept short to minimize the instability effect on reliability scores. This review did not seek to determine whether the intervals reported were appropriate, but rather documented the extent to which study authors reported they considered this issue or reported the time interval. Nine studies (Boyd and Dilley 2014; Boyd *et al.* 2012; Coppieters *et al.* 2009, 2015; Farooq 2012; Hough *et al.* 2000, 2007; Kasehagen *et al.* 2016; Martínez-Payá *et al.* 2015) did not report the specific intervals between measurement occasions.

#### *Reliability of ultrasound imaging measurements of nerve excursion*

Several types of statistics and plots have been recommended as the optimal indicators of the reliability of measurements performed using USI. These include intraclass correlation coefficients (ICCs), standard errors of measurement (SEMs), minimum detectable changes (MDCs) and Bland–Altman plots (Whittaker and Stokes 2011; Whittaker *et al.* 2007). Most of the studies included in this review used an ICC as the main reliability statistic, with the exceptions being use of a  $\kappa$  coefficient in one study (Martínez-Payá *et al.* 2015) and a dependability coefficient in another (Paquette *et al.* 2015), as noted in Table 3. Fourteen of the 18 studies reported an SEM, whilst 4 of the 18 studies reported a MDC. A majority of studies, 15 of 18, did not provide a Bland–Altman plot.

Table 3 provides details of the levels of reliability determined for the USI measurements of peripheral nerve excursion in each of the 18 included studies and for each nerve considered in the studies. Different types of reliability were assessed with 10 studies (Boyd and Dilley 2014; Boyd *et al.* 2012; Ellis *et al.* 2008, 2012; Filius *et al.* 2013; Hough *et al.* 2000, 2007; Kasehagen *et al.* 2016; Shum *et al.* 2013; Wang *et al.* 2014) examining intra-rater within-session reliability, 3 studies (Carroll *et al.* 2012; Paquette *et al.* 2015; Ridehalgh *et al.* 2012) examining intra-rater between-session reliability, 7 studies (Coppieters *et al.* 2009, 2015; Farooq 2012; Filius *et al.* 2013; Gonzalez-Suarez *et al.* 2015; Martínez-Payá *et al.* 2015; Wang *et al.* 2014)



Table 3. Reliability of ultrasound imaging measurements of peripheral nerve excursion

Inter-rater reliability	USI protocol	Study quality	Reported statistic	Reliability (ICC/ $\kappa$ coefficient/dependability coefficient; 95% CI; SEM; MDC/SRD [mm])				Bland-Altman plot	Nerve Level of evidence	
				Intra-rater reliability		Inter-rater reliability				
				Within session	Between sessions	Within session	Between sessions			
<b>Median nerve: Longitudinal movement</b>										
Gonzalez-Suarez et al. (2015)	Speckle tracking	Moderate	ICC				Distal arm = 0.91–0.93; 0.82–0.97; 0.02–0.03; 0.05–0.09 Wrist = 0.68–0.82; 0.37–0.91; 0.3–0.31; 0.82–0.86	Distal arm = 0.0–0.21; –0.95 to 0.59 Wrist = 0.64–0.78; 0.30–0.89	No	Median nerve = moderate
Paquette et al. (2015)	Speckle tracking	Moderate	Dependability coefficient		0.49–0.91 (ICC range); no 95% CI; 0.41–1.21 (SEM range); 0.95–2.82 (MDC range)			No		
Farooq (2012)	Speckle tracking	Moderate	ICC			0.96; no 95% CI; no SEM; no MDC		No		
Coppieters et al. (2009)	Speckle tracking	Moderate	ICC			0.96; 0.88–0.99; 0.66; 1.84		No		
Hough et al. (2007)	Spectral Doppler	Moderate	ICC	Elbow flexed = 0.95; 0.77–0.99; 0.32; no MDC Elbow extended = 0.89; 0.58–0.99; 0.49; no MDC				No		
Hough et al. (2000)	Spectral Doppler	Moderate	ICC	0.92; 0.87–0.96; 0.60; no MDC				No		
<b>Median nerve: Transverse movement</b>										
Martínez-Payá et al. (2015)	Nerve location comparison, start and end frames	Moderate	$\kappa$ coefficient				0.83; 0.69–0.97, no SEM; no MDC		No	
Wang et al. (2014)	Nerve location comparison, start and end frames	Moderate	ICC	0.91; 0.67–0.98, no SEM; no MDC			0.90; 0.60–0.98, no SEM; no MDC		No	
Filius et al. (2013)	Nerve location comparison, start and end frames	High	ICC	0.96; 0.85–0.99; no SEM; no MDC			0.98; 0.90–0.99; no SEM; no MDC		No	
Farooq (2012)	Speckle tracking	Moderate	ICC				0.92; no 95% CI; no SEM; no MDC		No	
<b>Median nerve: Superficial–deep movement</b>										
Martínez-Payá et al. (2015)	Nerve location comparison, start and end frames	Moderate	$\kappa$ coefficient				0.94; 0.83–1.00, no SEM; no MDC		No	
<b>Radial nerve: Longitudinal movement</b>										
Kasehagen et al. (2016)	Speckle tracking	High	ICC	Pronation with wrist flexion = 0.72–0.77 (range); 0.49–0.88; 0.19–0.48 (range); 0.53–0.80 (range) Pronation with wrist ulnar deviation = 0.85–0.86 (range); 0.71–0.93; 0.20–0.22 (range); 0.56–0.62 (range) Supination with wrist flexion = 0.76–0.79 (range); 0.56–0.88; 0.16–0.34 (range); 0.44–0.49 (range) Supination with wrist ulnar deviation = 0.63–0.70 (range); 0.36–0.84; 0.30–0.40 (range); 0.84–1.11 (range)					Yes	Radial nerve = limited
<b>Sciatic nerve: Longitudinal movement</b>										
Coppieters et al. (2015)	Speckle tracking	Moderate	ICC				0.97; 0.90–0.99; 0.94; no MDC		No	
Ridehalgh et al. (2012)	Speckle tracking	Moderate	ICC				Hip 30° flexion = 0.92; 0.79–0.97; 0.69; no MDC Hip 60° flexion = 0.96; 0.89–0.99; 0.87; no MDC		Yes	

(continued on next page)

Table 3. (continued)

Inter-rater reliability	USI protocol	Study quality	Reported statistic	Reliability (ICC/ $\kappa$ coefficient/dependability coefficient; 95% CI; SEM; MDC/SRD [mm])				Bland-Altman plot	Nerve Level of evidence
				Intra-rater reliability		Inter-rate reliability			
				Within session	Between sessions	Within session	Between sessions		
Ellis et al. (2012)	Speckle tracking	High	ICC	0.95; 0.92–0.96; 0.20; no MDC				No	
Ellis et al. (2008)	Speckle tracking	High	ICC	0.75; 0.59–0.87; 0.75; no MDC				Yes	
<b>Sciatic nerve: Transverse movement</b>									
Ellis et al. (2008)	Nerve location comparison, start and end frames	High	ICC	0.76; 0.60–0.87; 1.01; no MDC				No	
<b>Sciatic nerve: Superficial–deep movement</b>									
Ellis et al. (2008)	Nerve location comparison, start and end frames	High	ICC	0.39; 0.15–0.63; 0.62; no MDC				Yes	
<b>Tibial nerve: Longitudinal movement</b>									
Boyd and Dilley (2014)	Speckle tracking	Moderate	ICC	Knee = 0.87; 0.73–0.94; 0.21; no MDC Ankle = 0.87; 0.73–0.94; 0.33; no MDC				No	Tibial nerve = moderate
Shum et al. (2013)	Speckle tracking	Moderate	ICC	0.96; 0.93–0.98; 0.70; no MDC				No	
Boyd et al. (2012)	Speckle tracking	Fair	ICC	0.97; 0.94–0.99; 0.23; no MDC				No	
Carroll et al. (2012)	Speckle tracking	High	ICC	0.93; 0.70–0.96; 0.22–0.28 (range); 0.66–0.84 (range)				No	
Ellis et al. (2008)*	Speckle tracking	High	ICC	0.97; 0.73–0.99; 0.48; no MDC				No	
<b>Tibial nerve: Transverse movement</b>									
Boyd and Dilley (2014)	Speckle tracking	Moderate	ICC	Knee = 0.95; 0.89–0.98; 0.21; no MDC Ankle = 0.96; 0.92–0.98; 0.16; no MDC				No	
Boyd et al. (2012)	Speckle tracking	Fair	ICC	0.97; 0.94–0.99; 0.42; no MDC				No	
Ellis et al. (2008)	Nerve location comparison, start and end frames	High	ICC	0.70; 0.51–0.84; 1.38; no MDC				No	
<b>Tibial nerve: Superficial–deep movement</b>									
Boyd and Dilley (2014)	Speckle tracking	Moderate	ICC	Knee = 0.95; 0.89–0.98; 0.15; no MDC Ankle = 0.92; 0.83–0.96; 0.21; no MDC				No	
Shum et al. (2013)	Speckle tracking	Moderate	ICC	0.82; 0.68–0.92; 1.31; no MDC				No	
Boyd et al. (2012)	Speckle tracking	Fair	ICC	0.98; 0.96–0.99; 0.47; no MDC				No	
Ellis et al. (2008)	Nerve location comparison, start and end frames	High	ICC	0.56; 0.34–0.75; 0.85; no MDC				No	
<b>Common fibular nerve: Transverse movement</b>									
Boyd et al. (2012)	Speckle tracking	Fair	ICC	0.98; 0.95–0.99; 0.44; no MDC				No	Common fibular nerve =
<b>Common fibular nerve: Superficial–deep movement</b>									
Boyd et al. (2012)	Speckle tracking	Fair	ICC	0.98; 0.97–0.99; 0.34; no MDC				No	

USI = ultrasound imaging; PC = popliteal crease; PMT = posterior mid thigh; ICC = intra-class correlation coefficient; CI = confidence interval; SEM = standard error of measurement; MDC = minimal detectable change; SRD = smallest real difference.

\* This statistic was reported, but based on n = 3 participants.

examining inter-rater within-session reliability and 1 study (Gonzalez-Suarez et al. 2015) examining inter-rater between-session reliability. Comparisons between these different types of reliability was difficult as a majority of studies looked primarily at one form of reliability testing. One study compared within-session versus between-session inter-rater reliability (Gonzalez-Suarez et al. 2015), with reliability being less desirable for the between-session measures. Two studies (Filius et al. 2013; Wang et al. 2014) examined both intra-rater and inter-rater within-session reliability for the assessment of transverse movement of the median nerve, with comparable results.

Irrespective of the specific nerve imaged and the direction of excursion, the reliability of measurements of nerve excursion performed with USI was typically moderate to high. The exceptions to this finding were few. Paquette et al. (2015) reported a dependability coefficient of 0.49 (low reliability) for assessing median nerve excursion during a tensioner technique with the arm at 45° shoulder abduction. Ellis et al. (2008) reported an ICC of 0.39 (low reliability) for assessing superficial–deep (superficial = toward the skin, deep = away from the skin) sciatic nerve excursion at the posterior mid-thigh during a sliding technique performed at the ankle joint with the participants sitting.

#### *Level of evidence for the reliability of USI measurements of nerve excursion*

Consideration of the numbers of available studies and the methodological quality of each of those studies together (as per Table 1), along with the reliability findings described, revealed several findings regarding the levels of evidence that supported the key findings of this review. First, the pooled data, including all studies, nerves and directions of nerve excursion, provided a strong level of evidence to support the finding that the reliability of USI measurements of peripheral nerve excursion is typically moderate to high.

With respect to specific nerves assessed in included studies, the level of evidence to support the findings regarding reliability of USI measurements of excursion was found to be moderate for the median, sciatic and tibial nerves, and limited for the common fibular and radial nerves. Table 3 provides further details of the levels of evidence and USI reliability findings for each nerve.

## DISCUSSION

The current systematic review identified 18 published studies that have assessed the reliability of measurements of peripheral nerve excursion derived from USI. These 18 studies investigated five peripheral nerves, including the median, radial, sciatic, tibial and common

fibular nerves, across a variety of participant demographic characteristics.

One of the key aims of this review was to assess the methodological quality of those studies that have used USI as a method of quantifying nerve excursion. Across the 18 included studies, the methodological quality assessed via the MCAT was varied, with 4 studies of high, 13 studies of moderate and 1 study of low quality.

It should be noted that methodological limitations and specific measurement protocols may have directly influenced the levels of measurement reliability that were reported in the studies included in this review, and may also affect the reliability of such measurements in practice contexts. For example, it is widely accepted that USI is an operator-dependent tool. Therefore, the level of experience of the person who performs the USI may potentially influence the level of measurement reliability. The experience level of the sonographer has been reported to be positively associated with more consistent findings compared with less experienced examiners (Cartwright et al. 2013). Although not formally assessed from studies examining peripheral nerves with USI, differences in USI measurement reliability have been reported between experienced and novice sonographers when examining muscle morphology and function (Hides et al. 2007; Iwan et al. 2014). Eight of the included studies specifically described the experience level of the sonographer, whilst another three studies inferred that the sonographer had USI training. The remaining studies did not describe the sonographer.

The clear reporting of the experience level of the sonographer in future studies will be a key methodological feature to further increase confidence in findings regarding USI measurement reliability. Similarly, in practice contexts, the experience level of the sonographer and the extent to which the measurement protocol is both standardized and optimized will influence the precision of the measurements and the confidence we can have as to their accuracy.

Further inconsistencies in the reporting of methods included the description of observers/raters, particularly with respect to blinding, where 10 of the included studies failed to comment on this. Furthermore, the time between measurements was inconsistently reported. This may become a significant factor if the variable of interest (nerve excursion) has the capacity to change over time.

To facilitate the interpretation of reliability studies for USI measurements, experts in the field have advocated for optimization and consistency in both the statistical analyses used and the methods of reporting (Whittaker and Stokes 2011; Whittaker et al. 2007). Across the 18 studies included in this review, there was evidence of such consistency developing. For example, the majority of the included studies used statistics such as the ICC to report

their main reliability findings. Those that did not use the ICC instead used appropriate alternatives. However, there was variability in the use of supporting statistics, such as SEM, MDC, Bland–Altman plots and 95% confidence intervals.

It was clear from the review that few measurement protocols have been used to quantify nerve excursion from ultrasound data. By far, the majority of studies utilized speckle tracking via digital processing of specific grey-scale, speckle features between individual frames of an ultrasound video or cine loop. Although several different analysis methods were reported that utilized speckle tracking, the vast majority (12 of the 18 included studies) utilized the method reported by Dilley *et al.* (2001), and one study utilized the method reported by Nicoud *et al.* (2011). Two studies (Hough *et al.* 2000, 2007) reported the use of spectral Doppler USI to assess longitudinal median nerve movement. However, it was not apparent that this method has been utilized since 2007, with more contemporary studies preferring speckle-tracking protocols. It must be noted that more contemporary ultrasound methods, such as sonoelastography, are emerging as tools to examine nerve excursion (among other biomechanical parameters). Although these relevant studies did not meet inclusion for this review, it will be of interest to follow these emerging technologies.

Pooled data from the 18 studies yielded “strong” evidence that the reliability of USI measurements of peripheral nerve excursion is typically moderate to high, with few exceptions. This finding provides substantial support for the use of USI in clinical and healthy populations to measure peripheral nerve excursion. However, on a specific nerve basis, the levels of evidence vary, with a “moderate” level of evidence supporting the finding that the reliability of USI measurements of median, sciatic and tibial nerve excursion is, on balance, high to very high, but only “limited” evidence to support findings of very high reliability for USI assessment of the common fibular nerve and moderate to high reliability for the radial nerve. No published evidence was identified to elucidate the reliability of such measurements for other peripheral nerves. Differences in nerve anatomy, course through the body, depth and surrounding structures may all influence the ease (or lack of) for imaging certain nerves, which may influence the reliability of respective measurements. This highlights the need for further research to comprehensively examine the reliability of this measurement approach for those nerves for which limited or no evidence exists. Future research should consider the methodological weaknesses identified in the studies included in this review, which are evident in Table 2 and highlighted in the synthesis of key findings from the critical appraisal of included studies.

A number of possible benefits exist for quantifying nerve excursion in clinical practice. The technique may

be used as a diagnostic tool, for example, for the assessment of entrapment neuropathies (such as carpal tunnel syndrome) in which impaired nerve excursion is believed to be a key aetiological factor (Ellis *et al.* 2017). Furthermore, the selection of therapeutic techniques such as neural mobilization exercises, which aim to promote optimal peripheral nerve mechanics (Basson *et al.* 2017), may be better targeted to conditions where a known impairment of nerve movement against the interfacing tissues is identified with USI.

### *Strengths and limitations*

This review represents the first review we have been able to identify on this topic and, thus, valuably informs practice and future research. The strong levels of evidence for some key findings, particularly those indicating USI measurements of peripheral nerve excursion are typically reliable, ensure the review is valuable to practitioners and researchers alike. Researchers will also be usefully informed by the areas of the findings where the levels of evidence were limited or non-existent, as these gaps in the literature can inform research planning. Methodological deficiencies identified in the included studies can also usefully inform future research design.

The review has a number of limitations that must be acknowledged. First, a single reviewer conducted the initial literature search across all databases. Two reviewers appraised the identified articles for eligibility before critically appraising the selected articles, thus reducing human error and selection bias. Second, because the data from included studies were not amenable to meta-analysis because of the heterogeneity in, for example, methods, nerves examined and populations from which participants were drawn, the findings were synthesized using a critical narrative approach supported by descriptive quantitative analyses. Finally, it was accepted that there are many different methodological variables that can influence reliability. A pragmatic approach was taken for this review to present results in a manner in which an overall impression of the evidence was considered.

## CONCLUSIONS

The current systematic review identified a strong level of evidence to support the main finding that, typically, measurements of peripheral nerve excursion are moderately to highly reliable, with few exceptions. Although further research is needed to extend findings to nerves other than those examined in the included studies, the results of this review indicate that measurement of peripheral nerve excursion through USI is a promising technique that can be used with increasing confidence. Nevertheless, attention should be given to ensuring sonographer competence in the technique and ensuring the measurement protocols are

standardized and optimized. Further research is needed to build our knowledge of what optimization of these protocols should entail, to continue to explore the use of USI for such measurements in nerves other than those reported in this review and to further elucidate the clinical implications of different measurement values in varying clinical contexts and populations.

## REFERENCES

- Alshami AM, Cairns CW, Wylie BK, Souvlis T, Coppieters MW. Reliability and size of the measurement error when determining the cross-sectional area of the tibial nerve at the tarsal tunnel with ultrasonography. *Ultrasound Med Biol* 2009;35:1098–1102.
- Andrade RJ, Nordez A, Hug F, Ates F, Coppieters MW, Pezarat-Correira P, Freitas SR. Non-invasive assessment of sciatic nerve stiffness during human ankle motion using ultrasound shear wave elastography. *J Biomech* 2016;49:326–331.
- Barrett E, McCreesh K, Lewis J. Reliability and validity of non-radiographic methods of thoracic kyphosis measurement: A systematic review. *Man Ther* 2014;19:10–17.
- Basson A, Olivier B, Ellis R, Coppieters M, Stewart A, Mudzi W. The effectiveness of neural mobilization for neuro-musculoskeletal conditions: A systematic review and meta-analysis. *J Orthop Sports Phys Ther* 2017;47:593–615.
- Boyd BS, Dilley A. Altered tibial nerve biomechanics in patients with diabetes mellitus. *Muscle Nerve* 2014;50:216–223.
- Boyd BS, Gray AT, Dilley A, Wanek L, Topp KS. The pattern of tibial nerve excursion with active ankle dorsiflexion is different in older people with diabetes mellitus. *Clin Biomech (Bristol, Avon)* 2012;27:967–971.
- Brink Y, Louw QA. Clinical instruments: Reliability and validity critical appraisal. *J Eval Clin Pract* 2012;18:1126–1132.
- Carroll M, Yau J, Rome K, Hing W. Measurement of tibial nerve excursion during ankle joint dorsiflexion in a weight-bearing position with ultrasound imaging. *J Foot Ankle Res* 2012;5:5.
- Cartwright MS, Demar S, Griffin LP, Balakrishnan N, Harris JM, Walker FO. Validity and reliability of nerve and muscle ultrasound. *Muscle Nerve* 2013;47:515–521.
- Centre for Reviews and Dissemination. Systematic reviews: Centre for Reviews and Dissemination's guidance for undertaking reviews in health care. York: Author; 2009. University of York.
- Coppieters MW, Andersen LS, Johansen R, Giskegjerde PK, Hivik M, Vestre S, Nee RJ. Excursion of the sciatic nerve during nerve mobilization exercises: An in vivo cross-sectional study using dynamic ultrasound imaging. *J Orthop Sports Phys Ther* 2015;45:731–737.
- Coppieters MW, Hough AD, Dilley A. Different nerve-gliding exercises induce different magnitudes of median nerve longitudinal excursion: An in vivo study using dynamic ultrasound imaging. *J Orthop Sports Phys Ther* 2009;39:164–171.
- Dilley A, Greening J, Lynn B, Leary R, Morris V. The use of cross-correlation analysis between high-frequency ultrasound images to measure longitudinal median nerve movement. *Ultrasound Med Biol* 2001;27:1211–1218.
- Dilley A, Lynn B, Greening J, DeLeon N. Quantitative in vivo studies of median nerve sliding in response to wrist, elbow, shoulder and neck movements. *Clin Biomech (Bristol, Avon)* 2003;18:899–907.
- Dilley A, Odeyinde S, Greening J, Lynn B. Longitudinal sliding of the median nerve in patients with non-specific arm pain. *Man Ther* 2008;13:536–543.
- Dilley A, Summerhayes C, Lynn B. An in vivo investigation of ulnar nerve sliding during upper limb movements. *Clin Biomech (Bristol, Avon)* 2007;22:774–779.
- Ellis R, Hing W, Dilley A, McNair P. Reliability of measuring sciatic and tibial nerve movement with diagnostic ultrasound during a neural mobilization technique. *Ultrasound Med Biol* 2008;34:1209–1216.
- Ellis RF, Blyth R, Arnold N, Miner-Williams W. Is there a relationship between impaired median nerve excursion and carpal tunnel syndrome? A systematic review. *J Hand Ther* 2017;30:3–12.
- Ellis RF, Hing WA, McNair PJ. Comparison of longitudinal sciatic nerve movement with different mobilization exercises: An In vivo study utilizing ultrasound imaging. *J Orthop Sports Phys Ther* 2012;42:667–675.
- Farooq MN. Effects of whiplash injury on median nerve mobility: A comparative study. *J Physiother Sports Med* 2012;1:115–127.
- Filius A, Korstanje JW, Selles RW, Hovius SE, Slijper HP. Dynamic sonographic measurements at the carpal tunnel inlet: Reliability and reference values in healthy wrists. *Muscle Nerve* 2013;48:525–531.
- Fink A, Teggeler M, Schmitz M, Janssen J, Pisters M. Reproducibility of ultrasonographic measurements of the ulnar nerve at the cubital tunnel. *Ultrasound Med Biol* 2017;43:439–444.
- Gonzalez-Suarez C, Dizon JN, Cabungcal-Fidel B, Cua RCA, Dones VC, Lesniewski P, Thomas JC. Median nerve mobility measurement using a motion tracking analysis program: A reliability study. *Internet J Allied Health Sci Pract* 2015;13:4.
- Greening J, Dilley A. Posture-induced changes in peripheral nerve stiffness measured by ultrasound shear-wave elastography. *Muscle Nerve* 2017;55:213–222.
- Greening J, Dilley A, Lynn B. In vivo study of nerve movement and mechanosensitivity of the median nerve in whiplash and non-specific arm pain patients. *Pain* 2005;115:248–253.
- Hides JA, Miokovic T, Belavy DL, Stanton WR, Richardson CA. Ultrasound imaging assessment of abdominal muscle function during drawing-in of the abdominal wall: An intrarater reliability study. *J Orthop Sports Phys Ther* 2007;37:480–486.
- Hough AD, Moore AP, Jones MP. Peripheral nerve motion measurement with spectral Doppler sonography: A reliability study. *J Hand Surg Br* 2000;25B:585–589.
- Hough AD, Moore AP, Jones MP. Reduced longitudinal excursion of the median nerve in carpal tunnel syndrome. *Arch Phys Med Rehabil* 2007;88:569–576.
- Iwan T, Garton B, Ellis R. The reliability of measuring the inter-recti distance using high-resolution and low-resolution ultrasound imaging comparing a novice to an experienced sonographer. *NZ J Physiother* 2014;42:154–162.
- Kasehagen B, Ellis R, Mawston G, Allen S, Hing W. Assessing the reliability of ultrasound imaging to examine radial nerve excursion. *Ultrasound Med Biol* 2016;42:1651–1659.
- Martínez-Payá JJ, Ríos-Díaz J, del Baño-Aledo ME, García-Martínez D, de Groot-Ferrando A, Meroño-Gallut J. Biomechanics of the median nerve during stretching as assessed by ultrasonography. *J Appl Biomech* 2015;31:429–446.
- McDonagh C, Alexander M, Kane D. The role of ultrasound in the diagnosis and management of carpal tunnel syndrome: A new paradigm. *Rheumatology* 2015;54:9–19.
- Moher D, Liberati A, Tetzlaff J, Altman DG. Preferred reporting items for systematic reviews and meta-analyses: The PRISMA statement. *PLoS Med* 2009;6:e1000097.
- Nakamichi KI, Tachibana S. Restricted motion of the median nerve in carpal tunnel syndrome. *J Hand Surg Br* 1995;20B:460–464.
- Nicoud F, Castellazzi G, Lesniewski PJ, Thomas JC. Fast template tracking in video sequences. *Rev Sci Instrum* 2011;82:105–110.
- Paquette P, Lamontagne M, Higgins J, Gagnon DH. Repeatability and minimal detectable change in longitudinal median nerve excursion measures during upper limb neurodynamic techniques in a mixed population: A pilot study using musculoskeletal ultrasound imaging. *Ultrasound Med Biol* 2015;41:2082–2086.
- Prowse A, Pope R, Gerdhem P, Abbott A. Reliability and validity of inexpensive and easily administered anthropometric clinical evaluation methods of postural asymmetry measurement in adolescent idiopathic scoliosis: A systematic review. *Eur Spine J* 2016;25:450–466.
- Rabelo M, Nunes GS, Menezes da Costa Amante N, de Noronha M, Fachin-Martins E. Reliability of muscles strength assessment in chronic post-stroke hemiparesis: A systematic review and meta-analysis. *Top Stroke Rehabil* 2015;23:26–35.

- Ridehalgh C, Moore A, Hough A. Repeatability of measuring sciatic nerve excursion during a modified passive straight leg raise test with ultrasound imaging. *Man Ther* 2012;17:572.
- Ridehalgh C, Moore A, Hough A. Normative sciatic nerve excursion during a modified straight leg raise test. *Man Ther* 2014;19:59–64.
- Shum GL, Attenborough AS, Marsden JF, Hough AD. Tibial nerve excursion during lumbar spine and hip flexion measured with diagnostic ultrasound. *Ultrasound Med Biol* 2013;39:784–790.
- Topp KS, Boyd BS. Peripheral nerve: From the microscopic functional unit of the axon to the biomechanically loaded macroscopic structure. *J Hand Ther* 2012;25:142–152.
- van Tulder M, Furlan A, Bombardier C, Bouter L, Editorial Board of the Cochrane Collaboration Back Review Group. Updated method guidelines for systematic reviews in the Cochrane Collaboration Back Review Group. *Spine* 2003;28:1290–1299.
- Wang Y, Zhao C, Passe SM, Filius A, Thoreson AR, An KN, Amadio PC. Transverse ultrasound assessment of median nerve deformation and displacement in the human carpal tunnel during wrist movements. *Ultrasound Med Biol* 2014;40:53–61.
- Whittaker JL, Stokes M. Ultrasound imaging and muscle function. *J Orthop Sports Phys Ther* 2011;41:572–580.
- Whittaker JL, Teyhen DS, Elliott JM, Cook K, Langevin HM, Dahl HH, Stokes M. Rehabilitative ultrasound imaging: Understanding the technology and its applications. *J Orthop Sports Phys Ther* 2007;37:434–449.
- Yoshii Y, Tung WL, Ishii T. Measurement of median nerve strain and applied pressure for the diagnosis of carpal tunnel syndrome. *Ultrasound Med Biol* 2017;43:1205–1209.